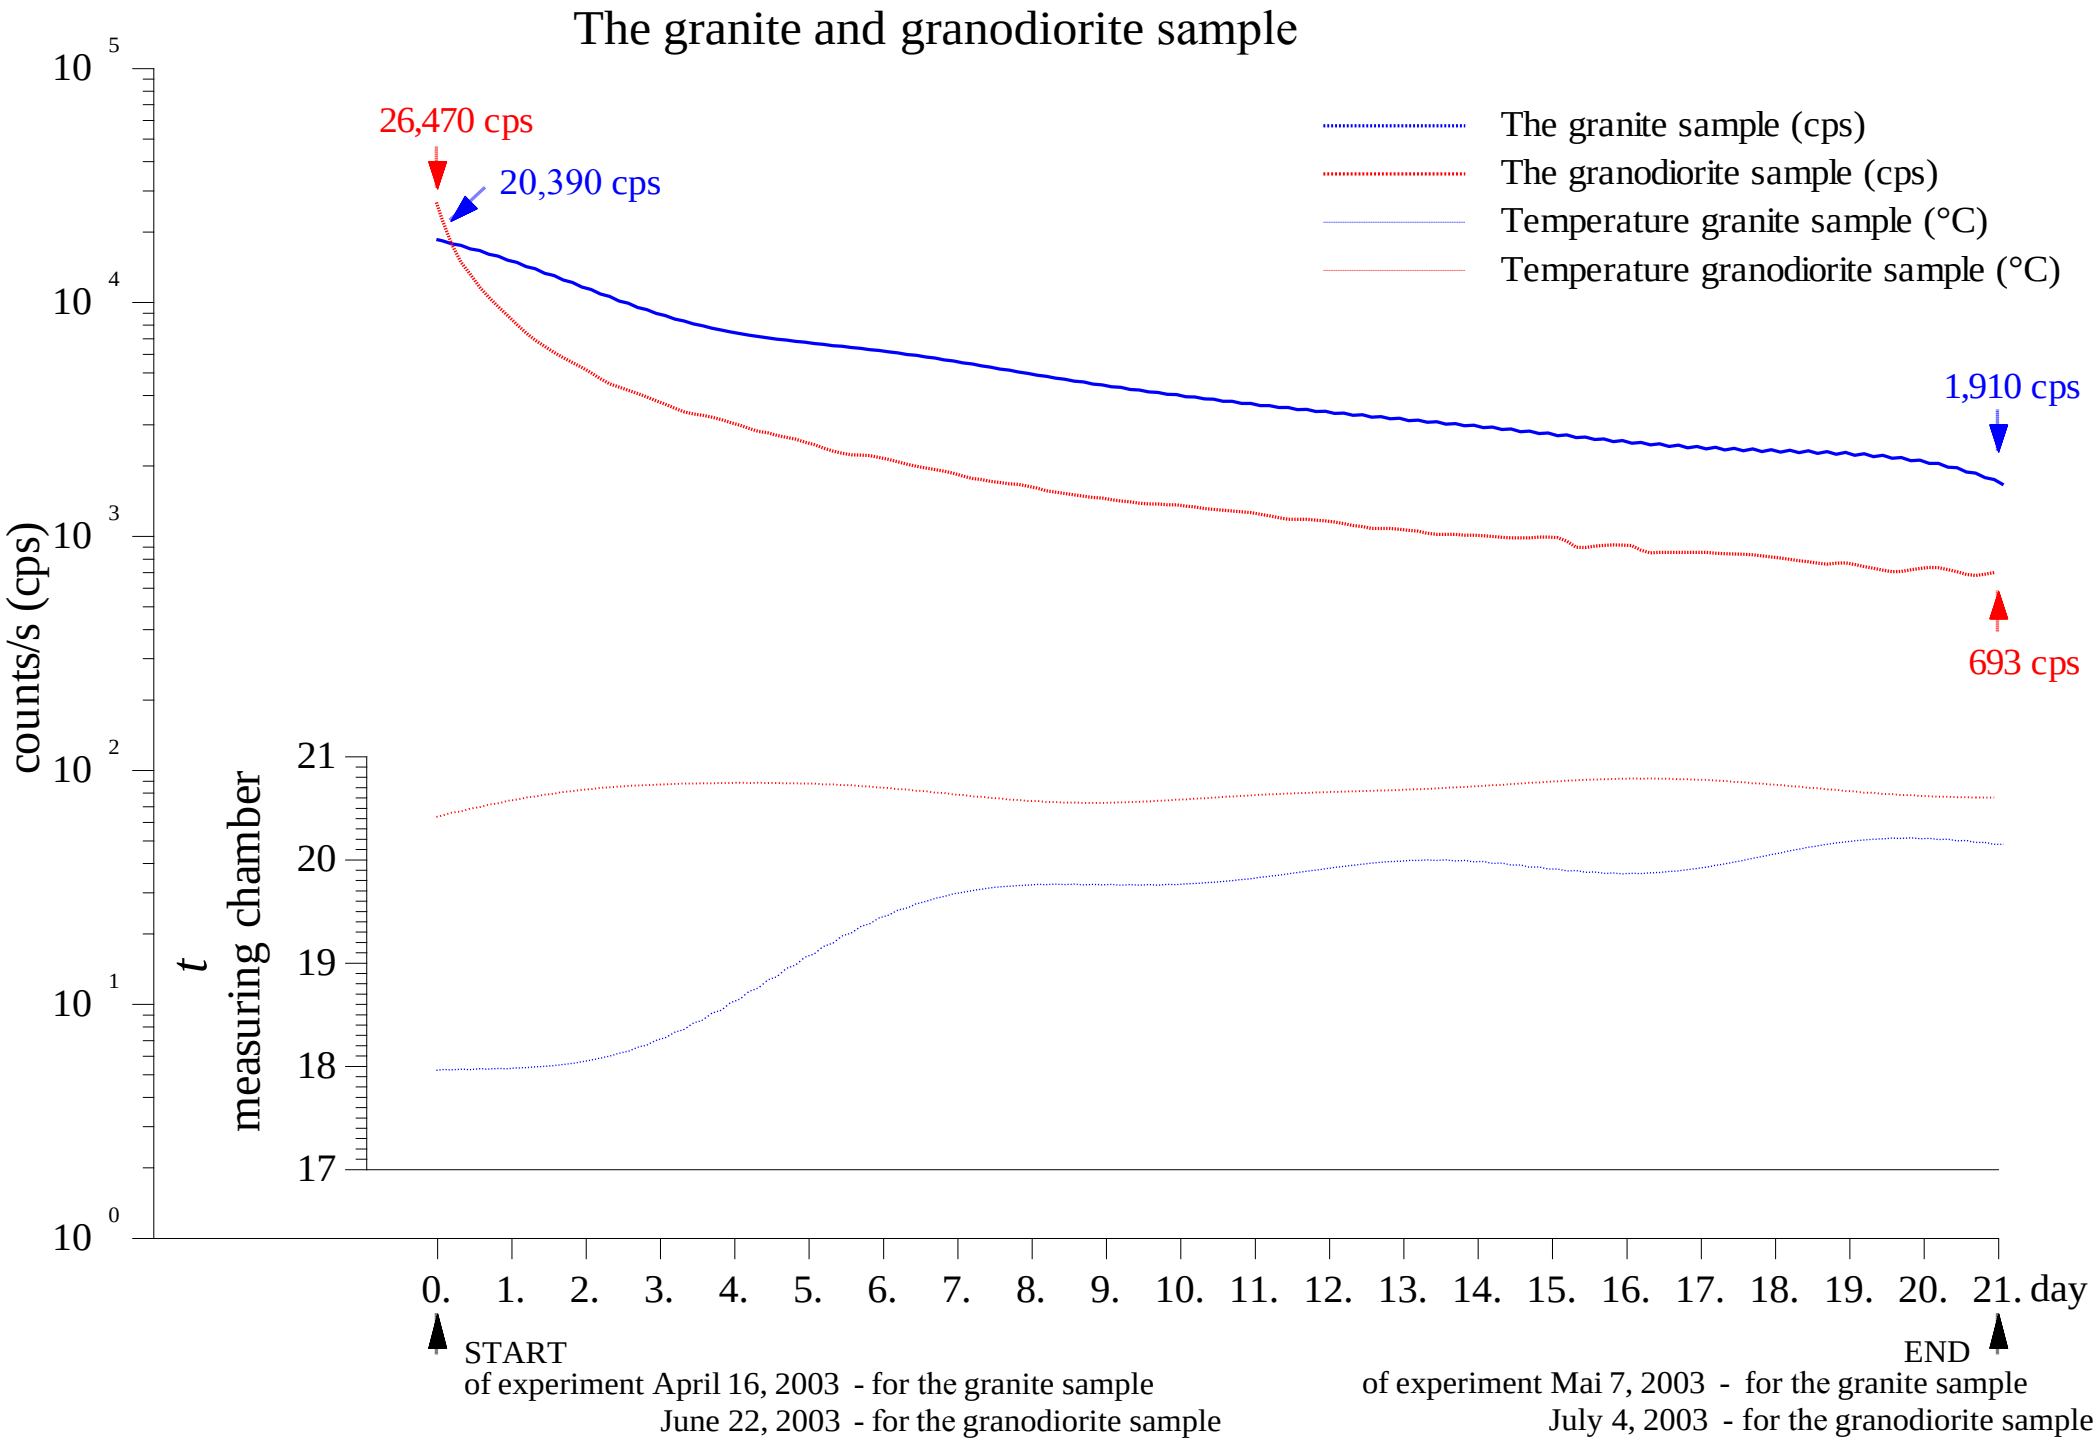
The granite and granodiorite sample
26,470 cps
20,390 cps
1,910 cps
693 cps
The granite sample (cps)
The granodiorite sample (cps)
Temperature granite sample (°C)
Temperature granodiorite sample (°C)
counts/s (cps)
t measuring chamber
0. 1. 2. 3. 4. 5. 6. 7. 8. 9. 10. 11. 12. 13. 14. 15. 16. 17. 18. 19. 20. 21. day
START
of experiment April 16, 2003 - for the granite sample
June 22, 2003 - for the granodiorite sample
END
of experiment Mai 7, 2003 - for the granite sample
July 4, 2003 - for the granodiorite sample